

Human Mitochondrial Open Reading Frame Of The 12S rRNA-c ELISA Kit (MOTS-c)

Catalog Number: RK01872

This ELISA kit used for quantitative determination of MOTS-c in human serum, plasma, tissue homogenates, cell lysates, cell culture supernates and other biological fluids. For research use only, and it's highly recommended to read thoroughly of this manual before using the product.

Manufactured by

Global Headquarters

500W Cummings Park

Ste. 6500 Woburn, MA 01801

Tel :888-754-5670

E-mail:info@abclonal.com

http: www.abclonal.com

China Branch

388# Gaoxin Road (No.2)

East Lake Development Zone

Wuhan P. R. China

Tel: 400-999-6126

E-mail: market@abclonal.com

http: www.abclonal.com.cn

Introduction

The kit is a competitive inhibition enzyme immunoassay technique for the in vitro quantitative measurement of MOTS-c in human serum, plasma, tissue homogenates, cell lysates, cell culture supernates and other biological fluids.

Principle of The Assay

This assay employs the competitive inhibition enzyme immunoassay technique. An antibody specific to MOTS-c has been pre-coated onto a microplate. A competitive inhibition reaction is launched between biotin labeled growth hormone and unlabeled MOTS-c (Standards or samples) with the pre-coated antibody specific to MOTS-c. After incubation the unbound conjugate is washed off. Next, avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. The amount of bound HRP conjugate is reverse proportional to the concentration of MOTS-c in the sample. After addition of the substrate solution, the intensity of color developed is reverse proportional to the concentration of MOTS-c in the sample.

Materials Provided

Part	Size (96T)	Cat NO.	STORAGE OF OPENED/ RECONSTITUTED MATERIAL
Antibody Coated Plate	8×12	RM03969	Return unused wells to the foil pouch containing the desiccant pack and store at ≤ -20 °C. Reseal along entire edge of zip-seal.
Standard Lyophilized	2	RM03970	Aliquot and store at ≤ -20 °C in a manual defrost freezer.* Avoid repeated freeze-thaw cycles.
Concentrated Biotin Conjugate Antigen Lyophilized	1	RM03971	May be stored for up to 6 month at -20 °C.*
Streptavidin-HRP Concentrated (100×)	1 ×120ul	RM03972	
Biotin-Conjugate Antigen reagent (R0)	1 ×300ul	RM00024A	May be stored for up to 6 month at 2-8 °C.*
Standard/Sample Diluent (R1)	1 ×20mL	RM00023	
Biotin Conjugate Antigen Diluent (R2)	1 ×12mL	RM00024	
Streptavidin-HRP Diluent(R3)	1 ×12mL	RM00025	
Wash Buffer(30x)	1 × 20mL	RM00026	
TMB Substrate	1 ×9 mL	RM00027	
Stop Solution	1 ×6 mL	RM00028	
Plate Sealers	4 strips		
Specification	1		

Storage Of The Kits

1. **For unopened kit:** All the reagents should be kept according to the labels on vials. Standard Lyophilized, Concentrated Biotin Conjugate Antigen Lyophilized, Streptavidin-HRP Concentrated and the Antibody Coated Plate should be stored at -20°C upon receipt while the others should be at 2-8 °C.
2. **For used kit:** When the kit is used, the remaining reagents need to be stored according to the above storage condition. Besides, please return the unused wells to the foil pouch containing the desiccant pack, and zip-seal the foil pouch.

Note:

It is highly recommended to use the remaining reagents within 1 month provided this is prior to the expiration date of the kit. For the expiration date of the kit, please refer to the label on the kit box. All components are stable up to the expiration date.

Sample Collection and Storage

1. Cell Culture Supernates:

Centrifuge 1000x g for 10 min and detect; or aliquot and store samples at -20°C to -70°C (Stored at 2-8°C if tested within 24 hours). Avoid freeze/thaw cycles. If cell culture supernate samples require larger dilutions, perform an intermediate dilution with culture media and the final dilution with the Standard/Sample Diluent(R1).

2. Serum:

Use a serum separator tube and allow samples to clot for two hours at room temperature or overnight at 4°C before centrifugation for 20 minutes at approximately 1,000xg. Assay freshly prepared serum immediately or store samples in aliquot at -20°C or -80°C for later use. Avoid repeated freeze/thaw cycles.

3. Plasma:

Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge samples for 15 minutes at 1,000xg at 2-8°C within 30 minutes of collection. Remove plasma and assay immediately or store samples in aliquot at -20°C or -80°C for later use. Avoid repeated freeze/thaw cycles.

4. Cell Lysates:

Cells need to be lysed before assaying according to the following directions. Adherent cells should be washed by cold PBS gently, and then detached with trypsin, and collected by centrifugation at 1,000 × g for 5 minutes (suspension cells can be collected by centrifugation directly). Wash cells three times in cold PBS. Resuspend cells in fresh lysis buffer with

concentration of 10^7 cells/ml. If it is necessary, the cells could be subjected to ultrasonication till the solution is clarified. Centrifuge at $1,500 \times g$ for 10 minutes at $2-8^\circ\text{C}$ to remove cellular debris. Assay immediately or aliquot and store at $\leq -20^\circ\text{C}$.

5. Tissue homogenates

The preparation of tissue homogenates will vary depending upon tissue type. Tissues were rinsed in ice-cold PBS to remove excess blood thoroughly and weighed before homogenization. Minced the tissues to small pieces and homogenized them in fresh lysis buffer (different lysis buffer needs to be chosen based on subcellular location of the target protein) (e.g. 1mL lysis buffer is added in 200mg tissue sample) with a glass homogenizer on ice (Micro Tissue Grinders works, too). The resulting suspension was sonicated with an ultrasonic cell disrupter till the solution is clarified. Then, the homogenates were centrifuged for 5 minutes at $10,000 \times g$. Collect the supernates and assay immediately or aliquot and store at $\leq -20^\circ\text{C}$.

6. Other biological fluids

Centrifuge samples for 20 minutes at $1,000 \times g$. Collect the supernates and assay immediately or store samples in aliquot at -20°C or -80°C for later use. Avoid repeated freeze/thaw cycles.

7. Avoid hemolytic and hyperlipidemia sample for Serum and Plasma.

8. Dilution:

Dilute samples at the appropriate multiple (recommend to do pre-test to determine the dilution factor).

Precautions

1. **FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.**
2. Any variation in diluent, operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.
3. Variations in sample collection, processing, and storage may cause sample value differences.
4. Reagents may be harmful, if ingested, rinse it with an excess amount of tap water.
5. Stop Solution contains strong acid. Wear eye, hand, and face protection.
6. Apart from the standard of kits, other components should not be refrigerated.
7. Please perform simple centrifugation to collect the liquid before use.
8. Do not mix or substitute reagents with those from other lots or other sources.
9. Adequate mixing is very important for good result. Use a mini-vortexer at the lowest frequency.
10. Mix the sample and all components in the kits adequately, and use clean plastic container to prepare all of the diluent.
11. Both the sample and standard should be assayed in duplicate, and the sequence of the reagents should be added consistently.
12. Reuse of dissolved standard is not recommended.
13. The kit should not be used beyond the expiration date on the kit label.
14. The kit should be away from light when it is stored or incubated.
15. To reduce the likelihood of blood-borne transmission of infectious agents, handle all serum, plasma and other biological fluids in accordance with

NCCLS regulations.


16. To avoid cross contamination, please use disposable pipette tips.
17. Please prepare all the kit components according to the Specification. If the kits will be used several times, please seal the rest strips and preserve with desiccants. Do use up within 2 months.
18. The 48T kit is also suitable for the specification.

Experiment Materials

1. Microplate reader (measuring absorbance at 450 nm, with the correction wavelength set at 570 nm or 630 nm).
2. Pipettes and pipette tips: 0.5-10, 2-20, 20-200, 200-1000 μ L.
3. Microplate washer, Squirt bottle.
4. Micro-oscillator.
5. Deionized or double distilled water, graduated cylinder.
6. Polypropylene Test tubes for dilution.
7. Incubator.

Reagent Preparation

- Bring all reagents to room temperature before use. If crystals have formed in the concentrate, Bring the reagent to room temperature and mix gently until the crystals have completely dissolved.**
- Standard:** Add Standard/Sample Diluent(R1) 1.0mL into freeze-dried standard, sit for a minimum of 15 minutes with gentle agitation prior to making dilutions (600ng/mL), Prepare EP tubes containing Standard/Sample Diluent(R1), and produce a dilution series according to the picture shown below (recommended concentration for standard curve: 200ng/mL, 66.67ng/mL, 22.22ng/mL, 7.41ng/mL, 2.47ng/mL). Redissolved standard solution (600ng/mL), aliquot and store at -20°C— -70°C.

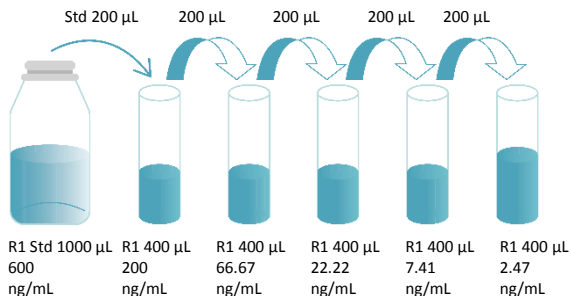

- 3. Concentrated Biotin Conjugate Antigen (100x):** Reconstitute the Biotin Conjugate Antigen with 150 μ L of Biotin-Conjugate Antigen reagent (R0), kept for 10 minutes at room temperature, shake gently(not to foam). Dilute to the working concentration with Biotin Conjugate Antigen Diluent (R2).

Dilution Method

Strip	Concentrated Biotin Conjugate Antigen (100x)	Biotin Conjugate Antigen Diluent (R2)
2	20ul	1980ul
4	40ul	3960ul
6	60ul	5940ul
8	80ul	7920ul
10	100ul	9900ul
12	120ul	11880ul

4. **Streptavidin-HRP Concentrated (100x):** Dilute 1:100 with the Streptavidin-HRP Diluent(R3) before use, and the diluted solution should be used within 30 min.

Dilution Method

Strip	Concentrated Streptavidin-HRP (100x)	Streptavidin-HRP Diluent(R3)
2	20ul	1980ul
4	40ul	3960ul
6	60ul	5940ul
8	80ul	7920ul
10	100ul	9900ul
12	120ul	11880ul

5. **Wash buffer:** Dilute 1:30 with double distilled or deionized water before use.

Wash Method


Aspirate each well and wash, repeating the process two times for a total of three washes. Wash by filling each well with **Wash Buffer**(300ul) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining **Wash Buffer** by aspirating or decanting. Invert the plate and blot it against clean paper towels.

Assay Procedure

1. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal.
2. Prepare the Biotin Conjugate Antigen Concentrated (100X) Working Solution 15 minutes early before use.
3. Add 50 μ L Standard/sample Diluent (R1) in blank well, add 50 μ L different concentration of standard and sample in other wells. And then add Biotin Conjugate Antigen Working Solution in each wells (50 μ L/well), cover with new adhesive strip provided. Incubate for 1 hour at 37°C.
4. Prepare the Streptavidin-HRP Concentrated (100X) Working Solution 15minutes early before use.
5. Remove the liquid of each well, Add wash buffer 350 μ L/well, aspirate each well after holding 60-120 seconds, repeating the process two times for a total of three washes.
6. Add Streptavidin-HRP Diluent(R3) in blank well and add Streptavidin-HRP Working Solution in other wells (100 μ L/well), cover with new adhesive strip provided. Incubate for 30 minutes at 37°C.
7. Warm-up the Microplate reader.
8. Remove the liquid of each well, Add wash buffer 350 μ L/well, aspirate each well after holding 60-120 seconds, repeating the process four times for a total of five washes.
9. Add TMB Substrate (90 μ L/well). Incubate for 15-20 minutes at 37°C .Protect from light.
10. Add Stop Solution (50 μ L/well), determine the optical density of each well within 5 minutes, using a Microplate reader set to 450 nm. If wavelength

correction is available, set to 570 nm or 630 nm. If wavelength correction is not available, subtract readings at 570 nm or 630 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.


Assay Procedure Summary

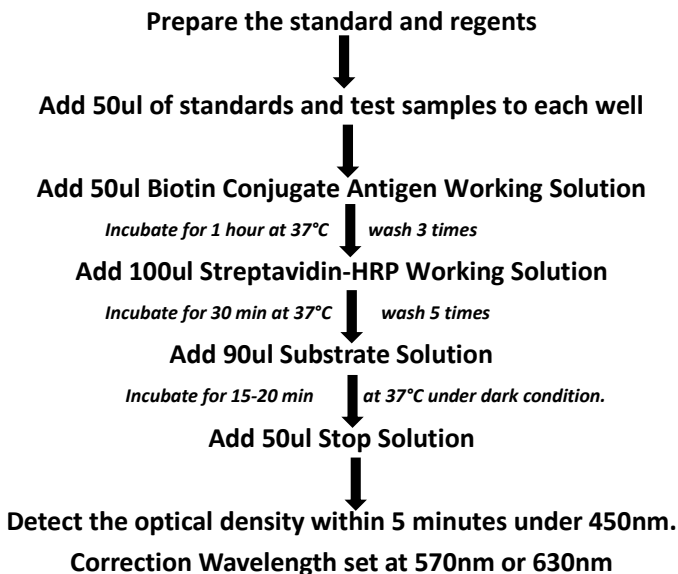

Calculation Of Results

1. In order to make the calculation easier, we plot the O.D. value of the standard (X-axis) against the log of concentration of the standard (Y-axis), although concentration is the independent variable and O.D. value is the dependent variable. The O.D. values of the standard curve may vary according to the conditions of assay performance (e.g. operator, pipetting technique, washing technique or temperature effects). Typical standard curve below is provided for reference only.
2. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

Typical Data

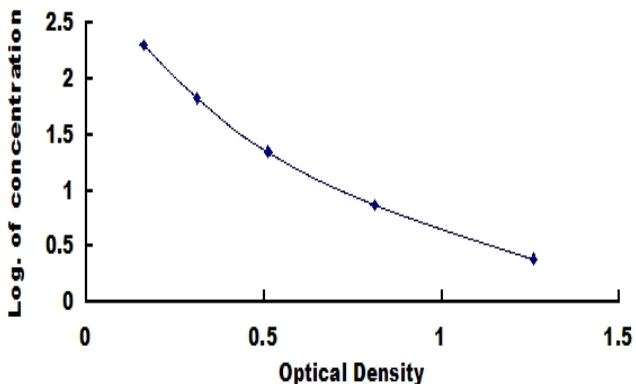

The standard curves are provided for demonstration only. A standard curve should be generated for each set of MOTS-c assayed.

Sensitivity

The minimum detectable dose (MDD) of MOTS-c is typically less than 0.94 ng/mL. The MDD was determined by adding two standard deviations to the mean optical density value of twenty zero standard replicates and calculating the corresponding concentration.

Specificity

This assay has high sensitivity and excellent specificity for detection of MOTS-c. No significant cross-reactivity or interference between MOTS-c and analogues was observed.

Note:

Limited by current skills and knowledge, it is impossible for us to complete the cross- reactivity detection between MOTS-c and all the analogues, therefore, cross reaction may still exist.

Precision

Intra-plate Precision

3 samples with low, middle and high level MOTS-c were tested 20 times on one plate, respectively.

Intra-Assay: CV<10%

Inter-plate Precision

3 samples with low, middle and high level MOTS-c were tested on 3 different plates, 8 replicates in each plate.

Inter-Assay: CV<12%

Recovery

Matrices listed below were spiked with certain level of MOTS-c and the recovery rates were calculated by comparing the measured value to the expected amount of MOTS-c in samples.

Matrix	Recovery range (%)	Average (%)
serum(n=5)	83-98	92
EDTA plasma(n=5)	78-91	86
heparin plasma(n=5)	95-105	101

Linearity

The linearity of the kit was assayed by testing samples spiked with appropriate concentration of MOTS-c and their serial dilutions. The results were demonstrated by the percentage of calculated concentration to the expected.

Sample	1:2	1:4	1:8	1:16
serum(n=5)	83-95%	81-98%	79-94%	85-96%
EDTA plasma(n=5)	80-97%	94-106%	84-99%	78-92%
heparin plasma(n=5)	92-105%	89-102%	87-101%	80-93%